



## VILLA LABECO, s.r.o.


Chrapčiakova 1, 052 01 SPIŠSKÁ NOVÁ VES, SLOVAKIA

tel.: 00421 53 44 260 32 fax : 00421 53 4298359

email: [info@villalabeco.sk](mailto:info@villalabeco.sk), [www.villalabeco.sk](http://www.villalabeco.sk)

## HV power supply for electrophoresis

Programmable HV power supply for electrophoretic and relative techniques provide HV up to 30 kV at 300 microampers ( standard) or 20 kV with max. current 500  $\mu$ A ( this model for special request). All parameters : current, voltage and polarity are set via simple and friendly use keyboard. Constant voltage or constant current operation.

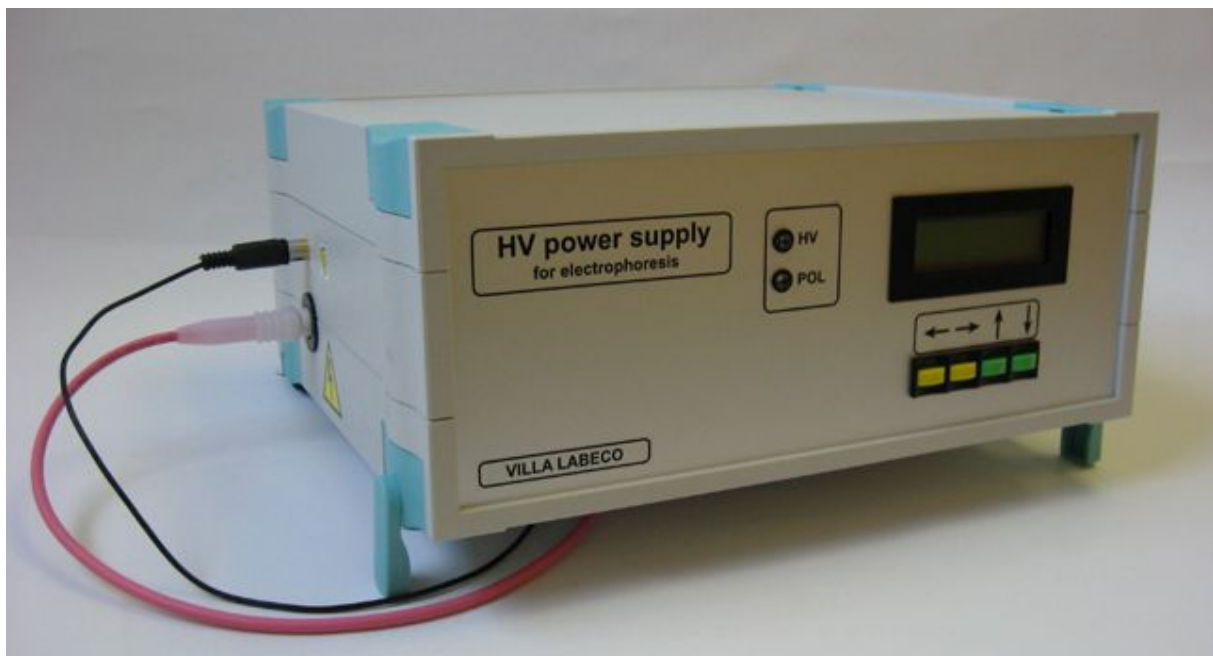

**Spellman Inside!**

### Parameters :

Max. voltage	30 ( resp. 20 ) kV	Input	24 V DC
Max. current	300 (resp.500) microampers	Step time	0-600 s
Min. progr. step	1 microamper/20V	Weight	5,5 kg
Size	320 x 220 x 170 mm (w x d x h)		

**Price : 1950.- EUR**